



University of **HUDDERSFIELD**

University of Huddersfield Repository

Gao, F., Jiang, Xiang, Muhamedsalih, Hussam and Martin, Haydn

Wavelength Scanning Interferometry for Thin Film Analysis of Fusion Target

Original Citation

Gao, F., Jiang, Xiang, Muhamedsalih, Hussam and Martin, Haydn (2010) Wavelength Scanning Interferometry for Thin Film Analysis of Fusion Target. In: 3rd European Target Fabrication Workshop, 30 September-1 October, Oxford. (Unpublished)

This version is available at <http://eprints.hud.ac.uk/id/eprint/9072/>

The University Repository is a digital collection of the research output of the University, available on Open Access. Copyright and Moral Rights for the items on this site are retained by the individual author and/or other copyright owners. Users may access full items free of charge; copies of full text items generally can be reproduced, displayed or performed and given to third parties in any format or medium for personal research or study, educational or not-for-profit purposes without prior permission or charge, provided:

- The authors, title and full bibliographic details is credited in any copy;
- A hyperlink and/or URL is included for the original metadata page; and
- The content is not changed in any way.

For more information, including our policy and submission procedure, please contact the Repository Team at: E.mailbox@hud.ac.uk.

<http://eprints.hud.ac.uk/>

Wavelength Scanning Interferometry for Thin Film Analysis of Fusion Targets

F. Gao, X. Jiang, H. Muhamedsalih and H. Martin

Centre for precision technologies

University of Huddersfield

Huddersfield, UK

3rd European Target Fabrication Workshop, 20th September -1st October 2010 Oxford, UK

Outline

- Review on thin film measurement
- Introduction to Scanning Wavelength Interferometry (SWI)
- Scanning Wavelength Interferometry for thin film measurement
- Experiments on films of fusion target
- Measurement results comparison
- Looking forward

Review of thin film measurement

- Methods and instruments used for thin film measurements


- Established methods

- Spectrophotometry
 - Ellipsometry
 - Scanning White Light Interferometry

- Methods used in research

- Wavelength Scanning Interferometry
 - Thermal-wave detection with laser beam deflection
 - Prism coupler
 - SEM for measuring metal film

Wavelength scanning interferometry

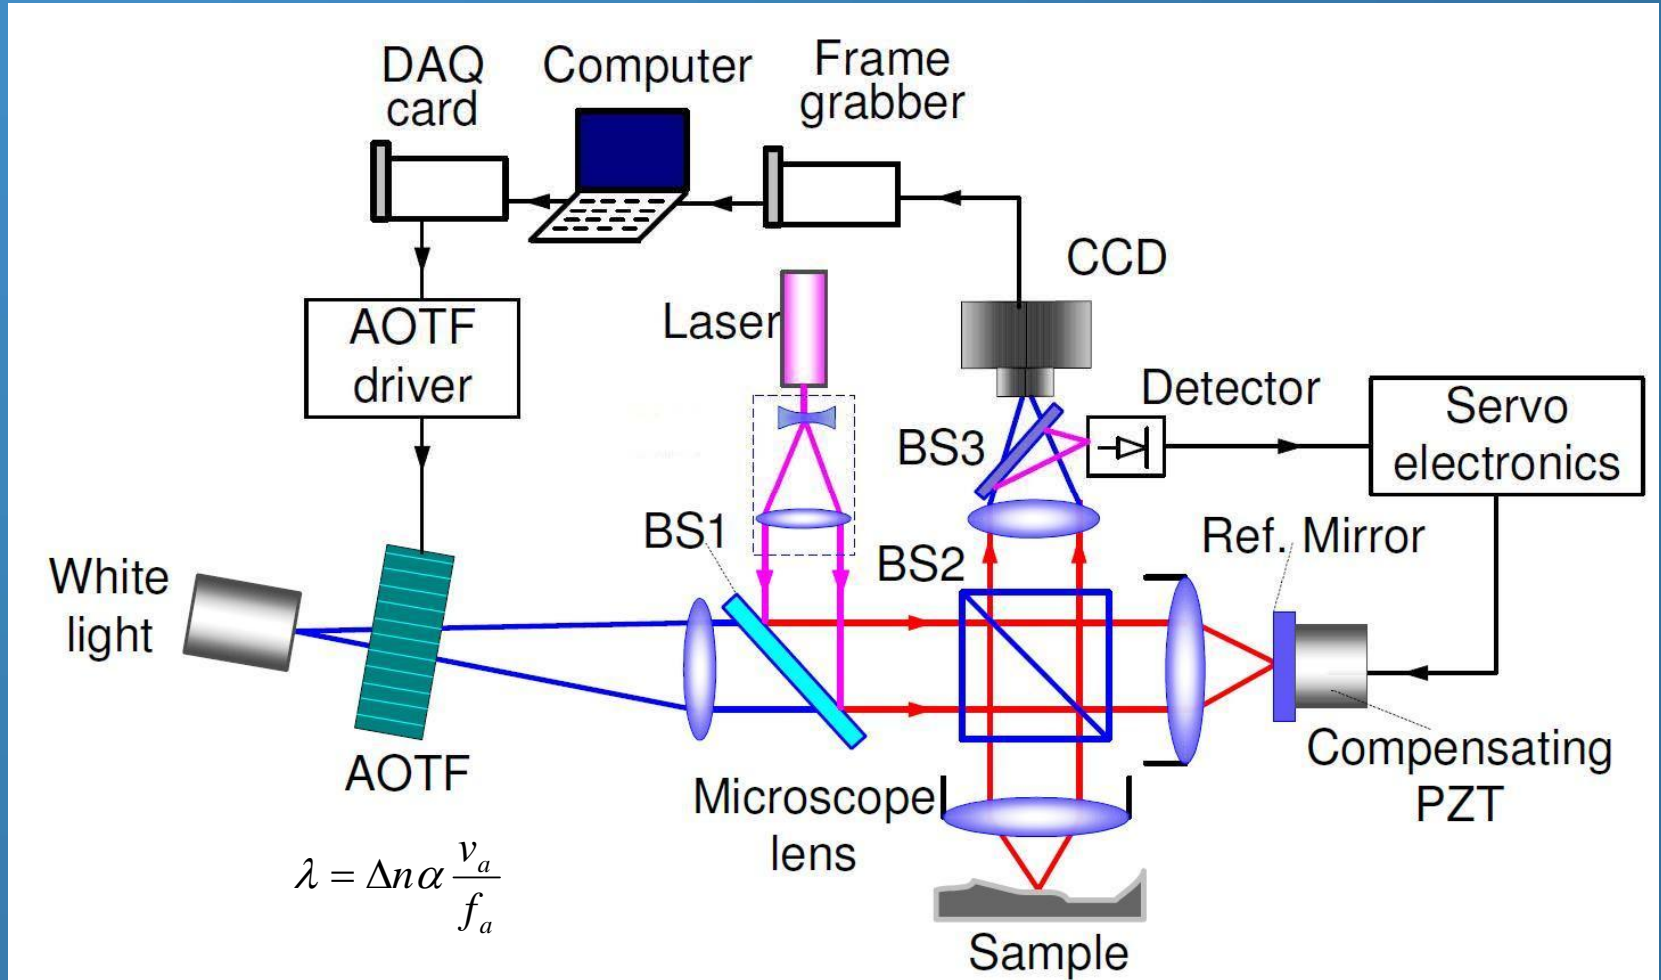

Optical setup

1. Linnik interferometer was used for the measurement.
2. AOTF has been employed to shift the wavelength from 680.8nm to 529.8nm. A series of interferograms were obtained.



Intensity Pattern at each pixel in the CCD

- DC component
- Cosine term
- High frequency Noise

$$I(i) = I_1 + I_2 + 2\sqrt{I_1 I_2} \cos(\phi(i)) \quad \text{where} \quad \phi(i) = \frac{2\pi}{\lambda(i)} * 2 * t$$

Analyze the intensity interferograms


- Convolution
- FFT

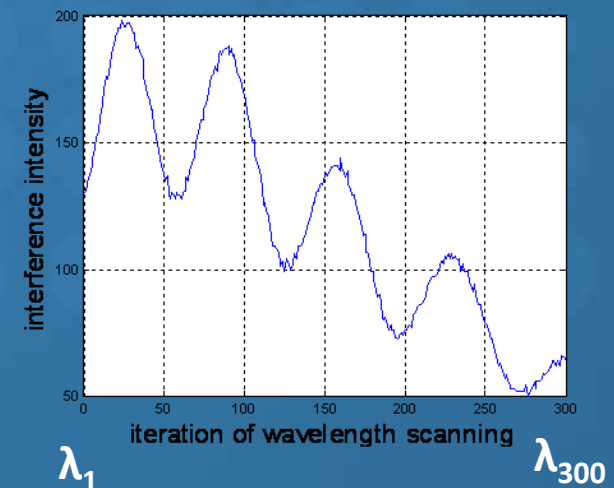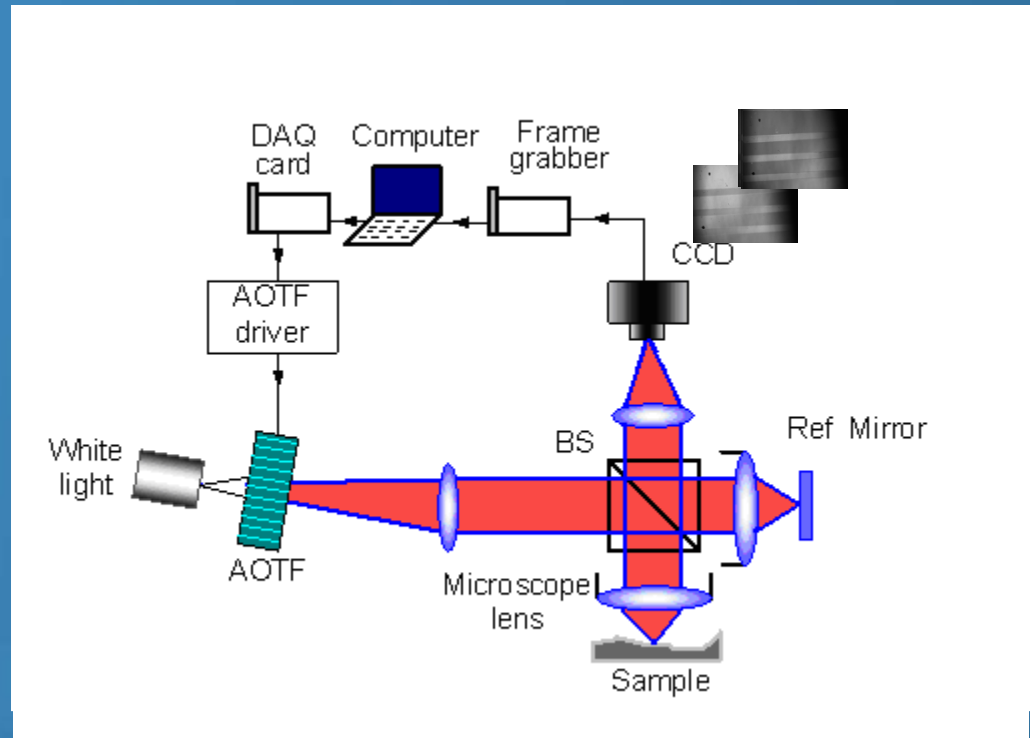

Calculation of the OPD

$$I(x, y, k) = A(x, y, k) + B(x, y, k) \cos(\varphi(x, y, k))$$

Phase change of π

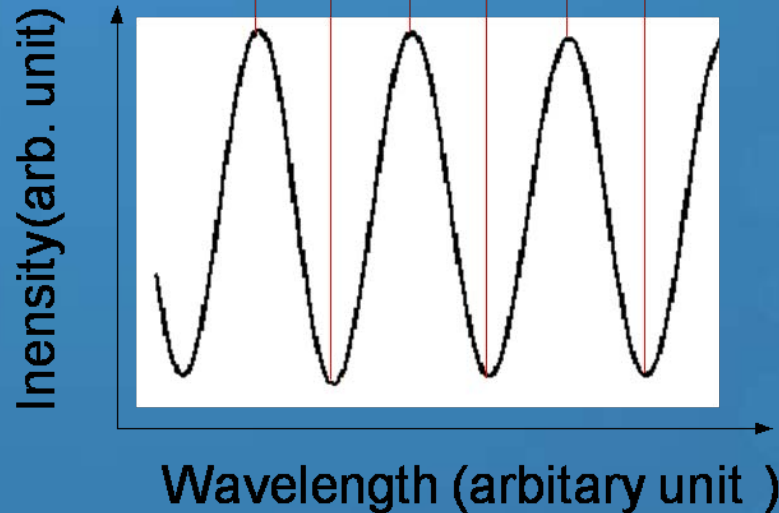


$$\varphi(x, y, k) = kh(x, y) = \frac{4\pi}{\lambda} h(x, y)$$

Phase Wave number Height


$$\Delta \varphi(x, y, \Delta k) = \Delta kh(x, y)$$

$$h(x, y) = \frac{\Delta \varphi(x, y, \Delta k)}{\Delta k}$$


System configuration

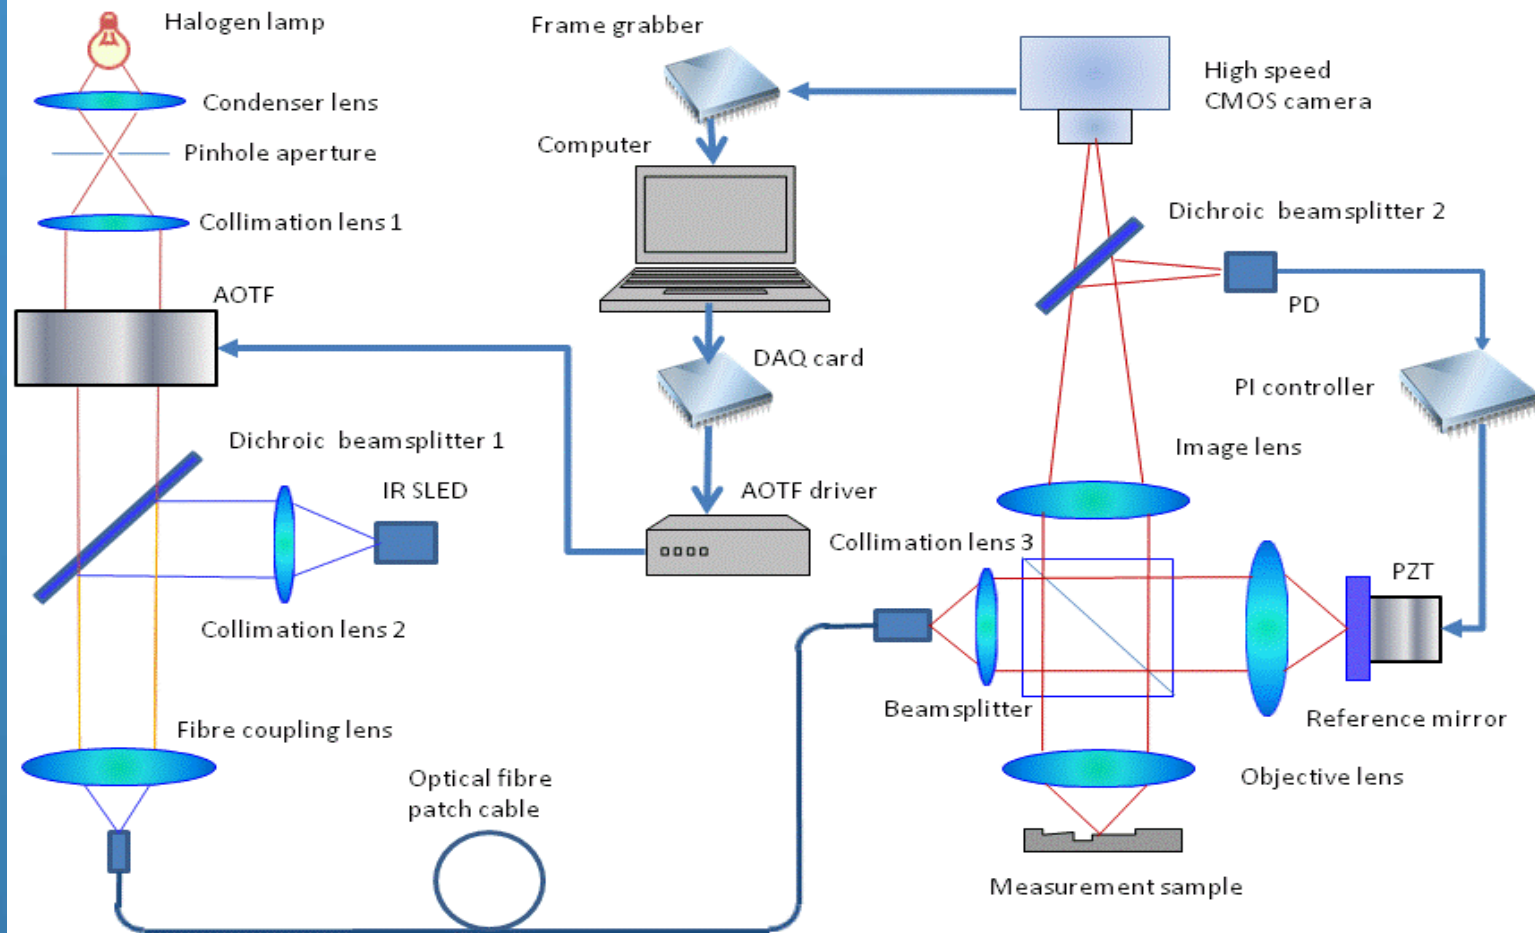




Experimental set up

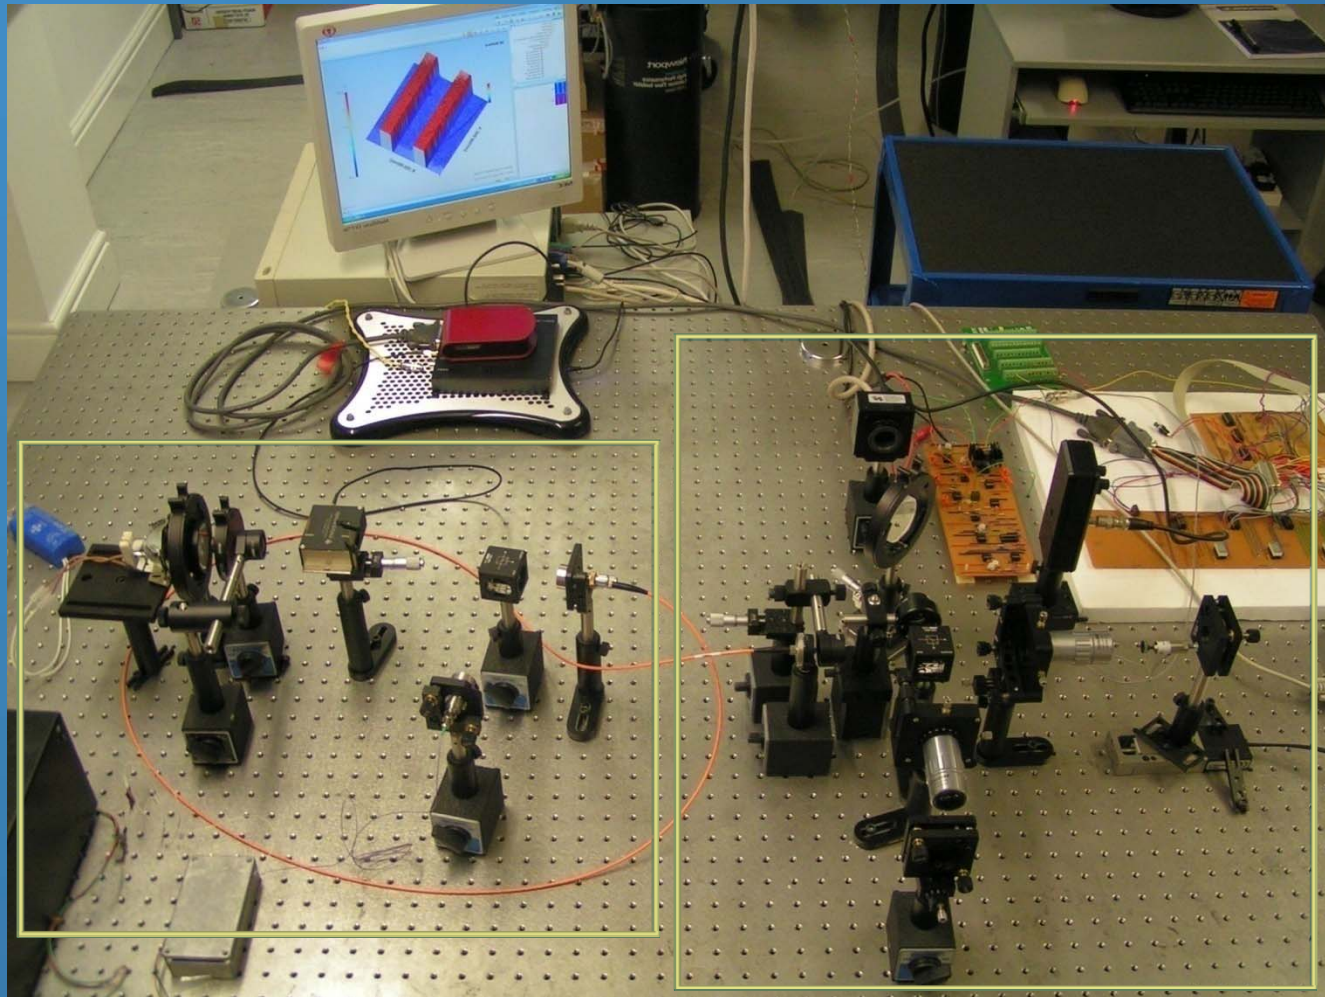

Measurements on step height standards

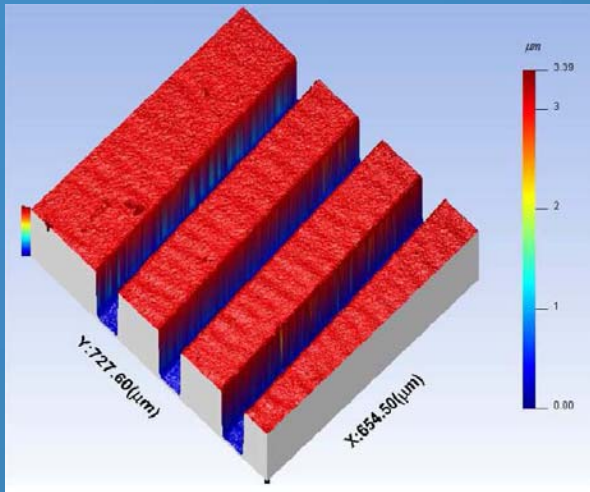

A 2.970 μm step height standard with uncertainty 1nm National Physical Laboratory (NPL)

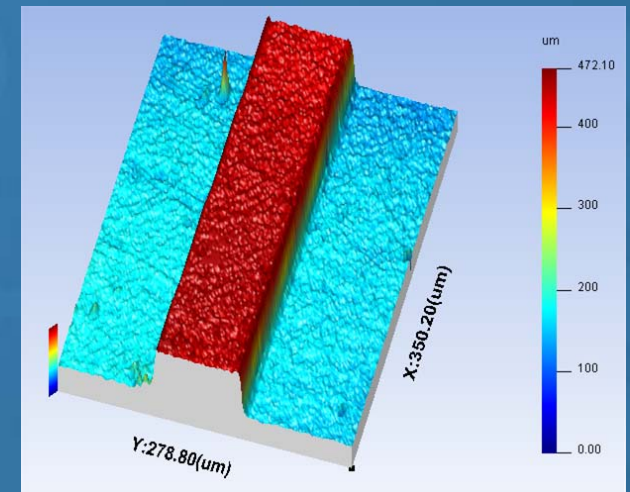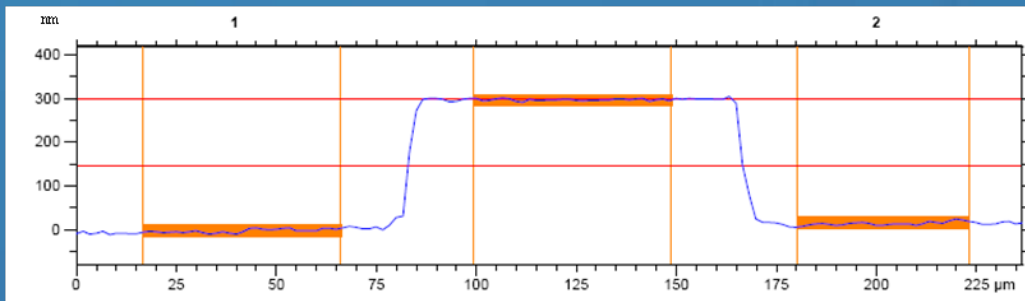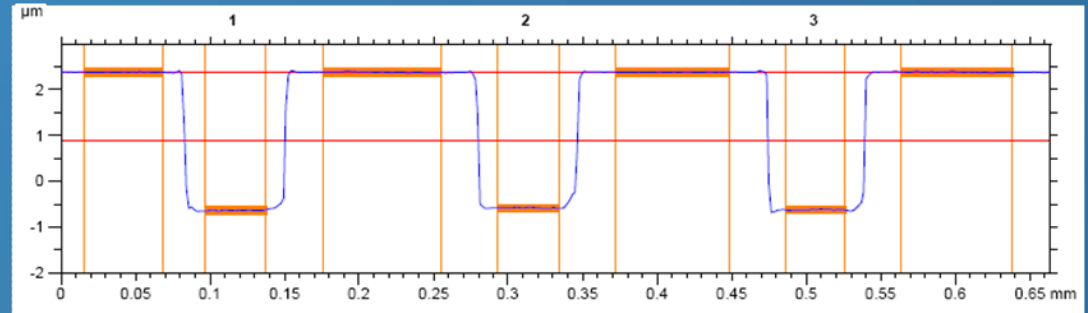

A 292 nm step height standard with uncertainty 0.9nm
Physikalisch-Technische Bundesanstalt (PTB)


Stabilisation

Stabilize Linnik Interferometer

The PZT has been attached to the reference mirror to compensate for the environmental disturbances.


The environmental vibration is fed back to servo electronics that contains PI controller to control PZT movement

The noise effect on the interferometer has been reduced 13.4dB

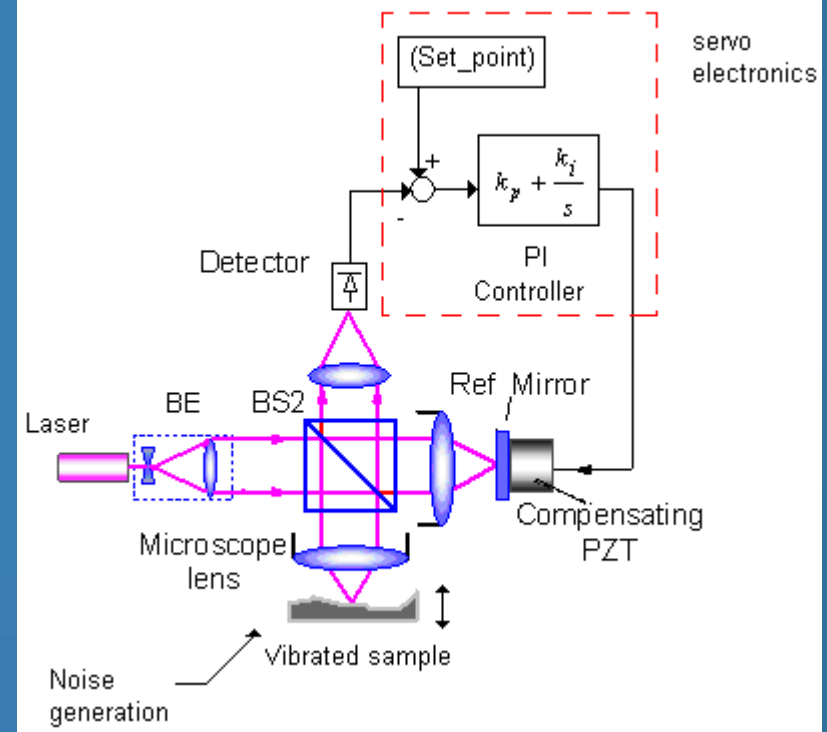


2V peak to peak and random frequency < 1KHz


Before
stabilization

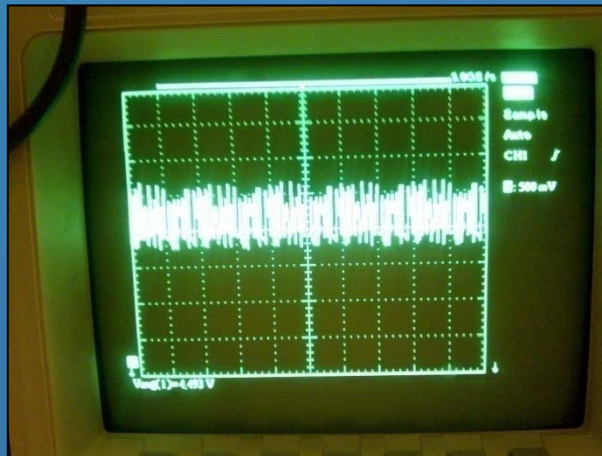


After
stabilization

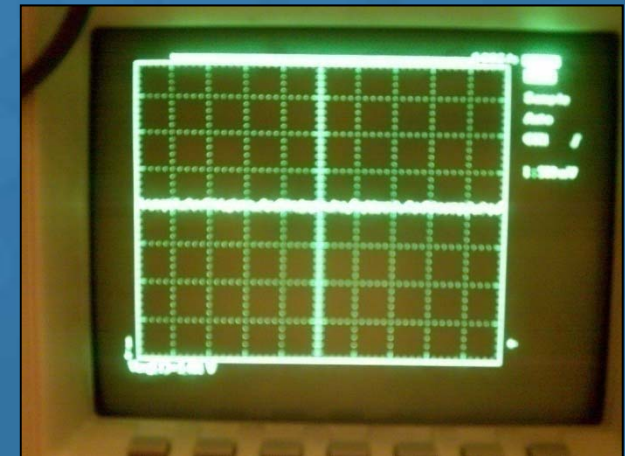


Anti vibration tests

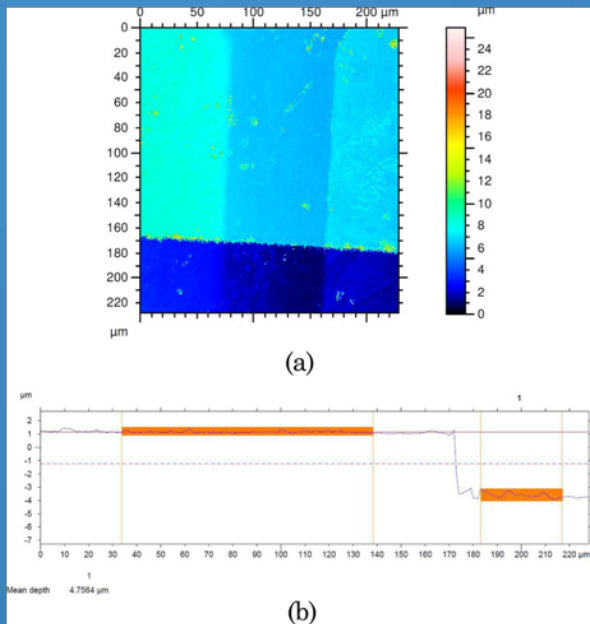

A semiconductor chip sample was measured without inducing mechanical disturbance. The measured surface step height is **4.7564 μm**

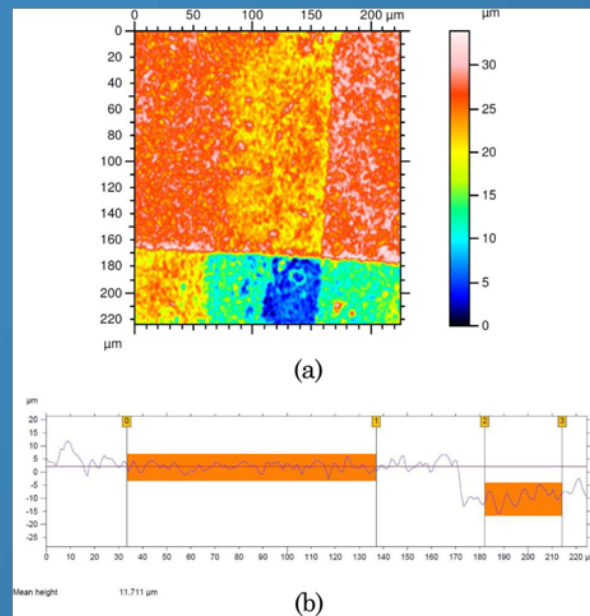

A 40 Hz and 400 nm peak-to-peak sinusoidal mechanical disturbance using a PZT was applied to the reference mirror. During the disturbance, the measured surface step height is **11.711 μm** .

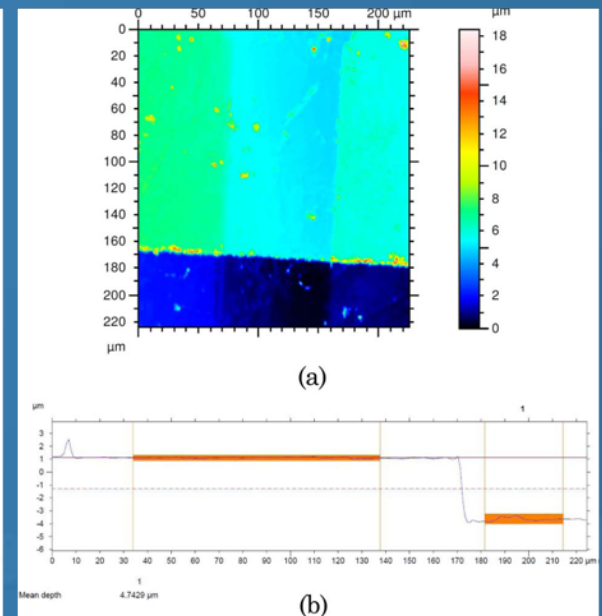




The measured step height is **4.7429 μm** when the vibration compensation system is on and 40 Hz 400 nm disturbance is applied.

Imaging processing using GPU

- A distinct advantage of the GPU technology compared to the CPU is that the GPU can process the images frame by frame while the CPU processes the images pixel by pixel.
- The GeForce GTX 280 with 240 cores has been used.
- The computing time has been reduced from 31.4 seconds to below a second.

The SWI was designed for Structured surfaces Measurement


Typical structured elements	Pitch lengths (μm)	Depths (μm)	Angles ($^\circ$)
V-grooves/Pyramid	14-141 (most 35-106)	10-100 (most 25-75)	45
Micro lens	30-100	3-20	
Diffraction lens	25-180	1-60	A=70-89 B =0 –10

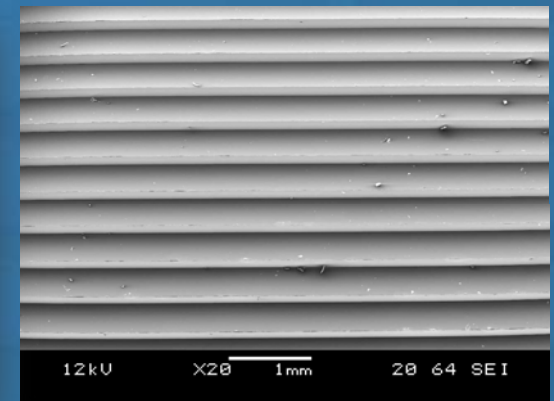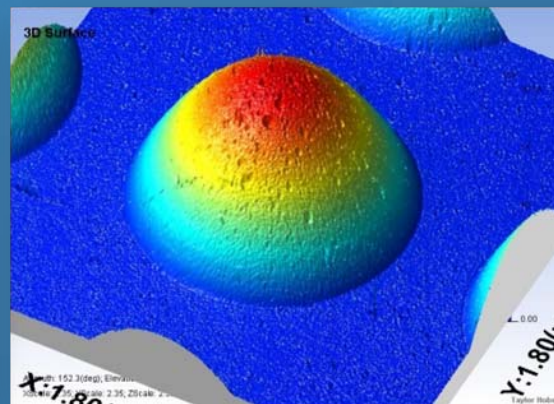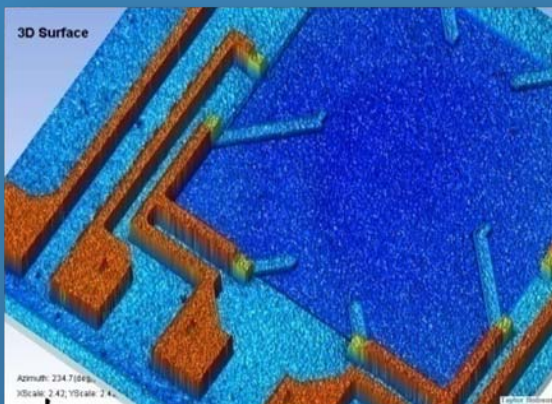

SWI for thin film measurement



- SWI can be used for thin film measurement.
- The two surfaces of the film can be used as the two mirrors of an interferometer to measure the thickness of the film.
- Using the configuration of our SWI system the surface information of both top surface of the film and the surface of substrate maybe extracted from the interference signals.

The flow chart of the analysis

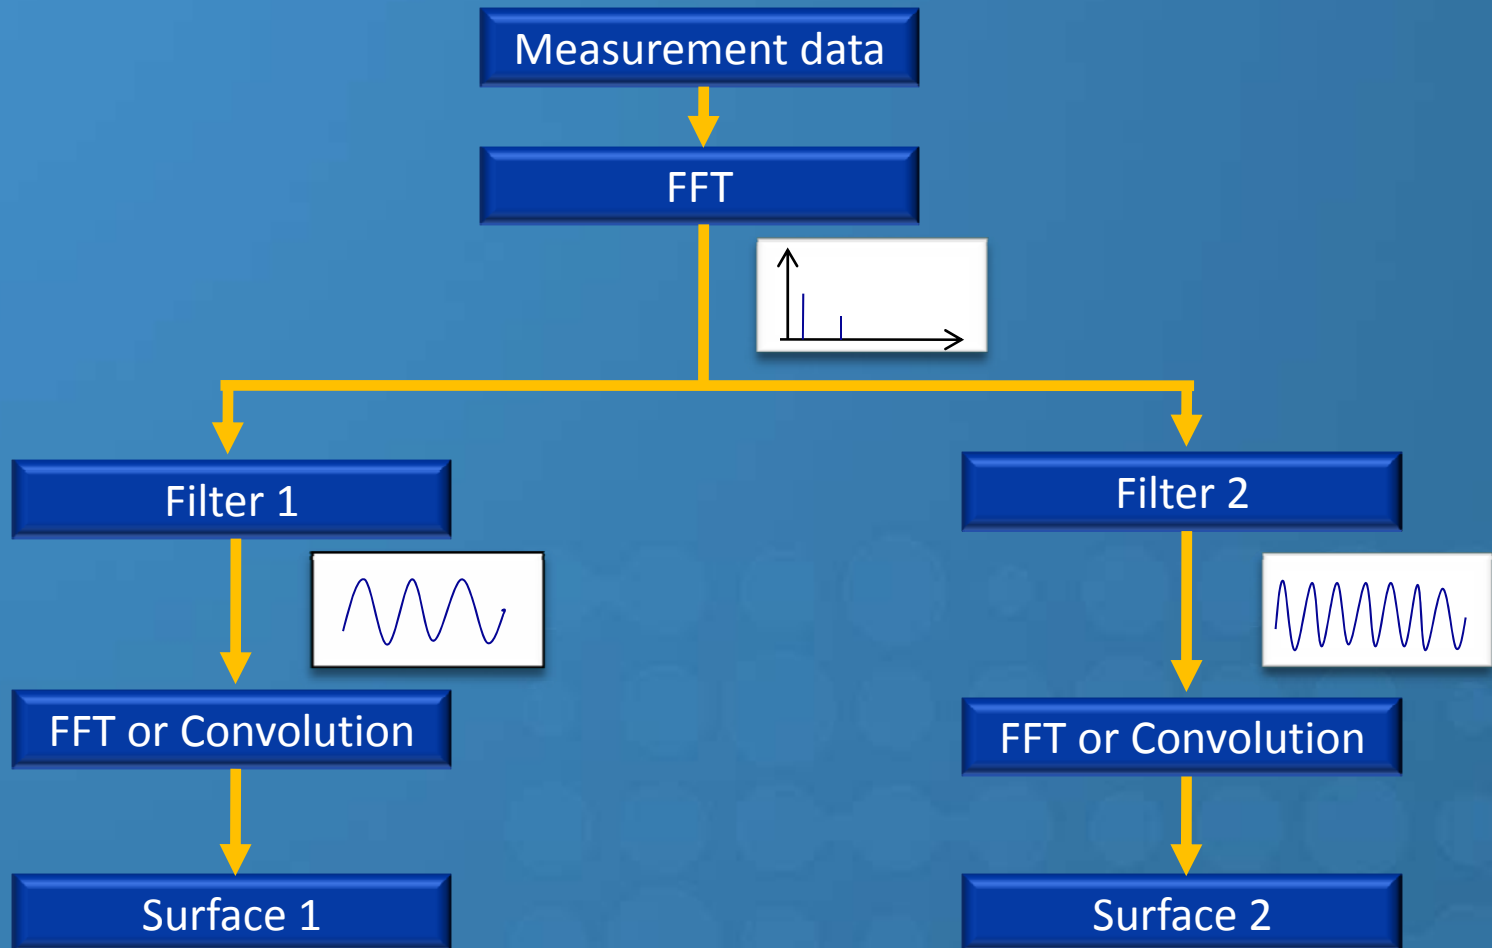




Simulation study of the measurement on a 10um film surfaces

- Bottom left - Three simulated interference signals generated between the reference mirror and the top surface, the reference mirror and bottom surface and between the two film surfaces
- Bottom right - Simulated combined signal on CCD camera

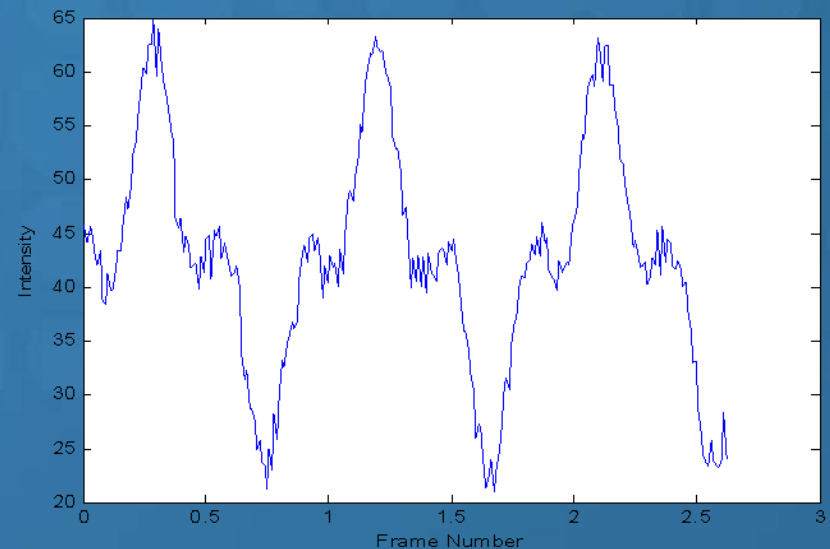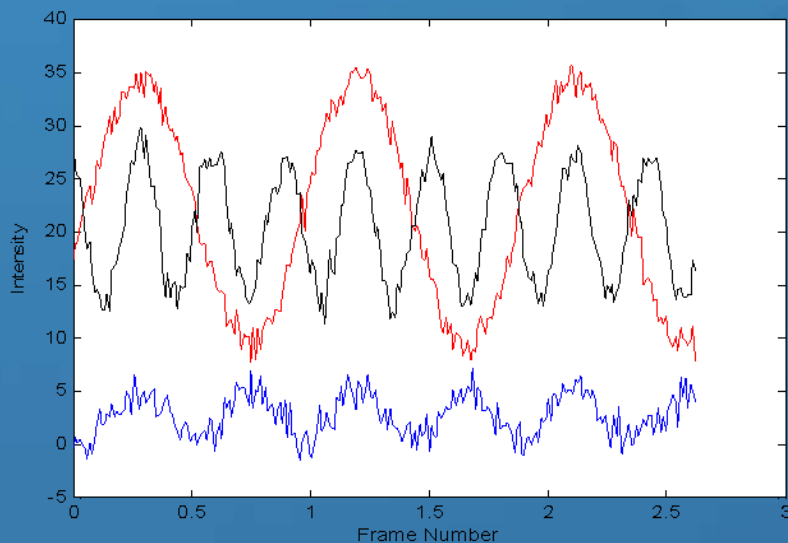



FFT analysis on the simulated signals

- Apply FFT analysis to find out the frequency components of the measured signal (top right)
- Construct filters according to the FFT analyse result
- Re-construct the two film surfaces (middle right and bottom right)

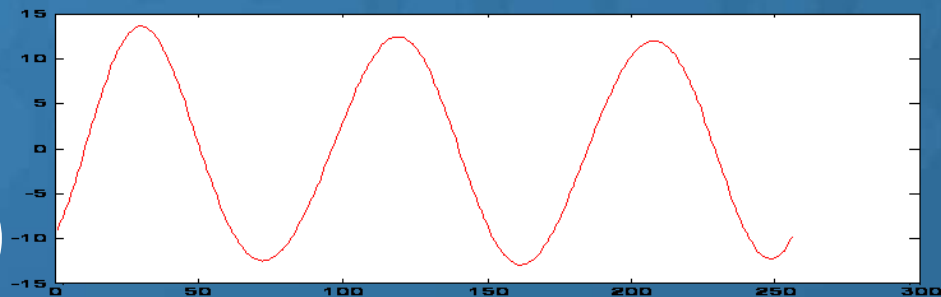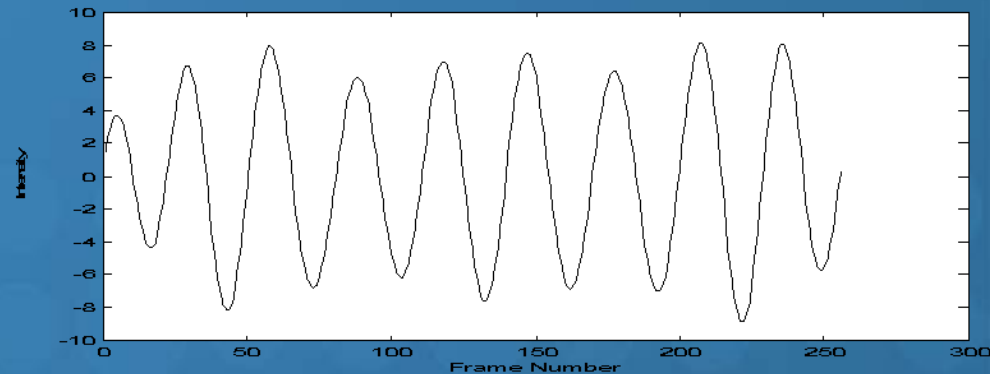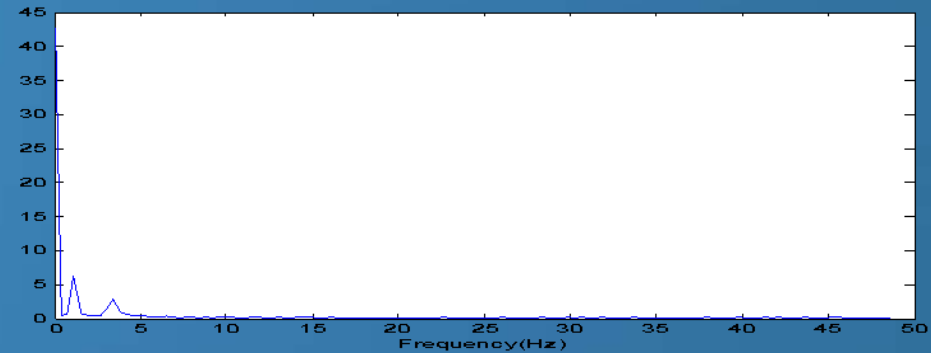



Real measurement signals on 10um film

- Top right - Measured interference fringe
- Middle right - measured interferogram signal on film coated area
- Bottom right – Measured interferogram of glass substrate

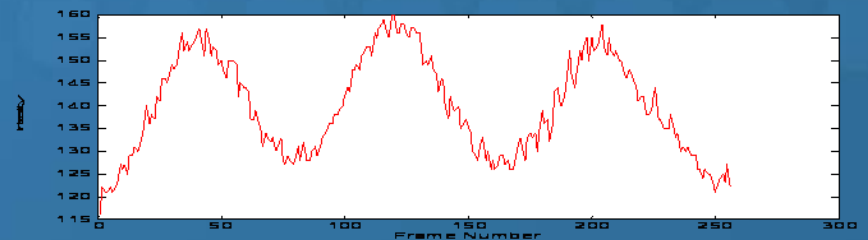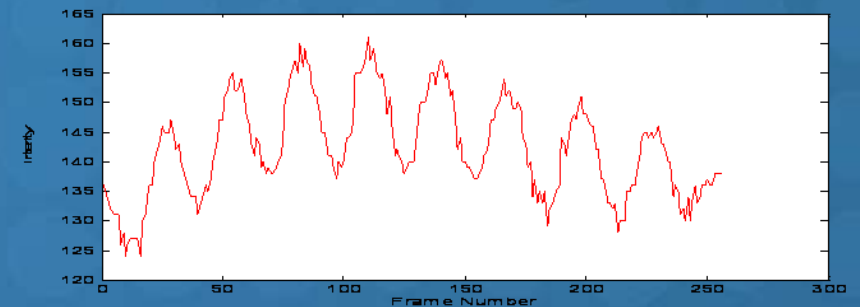

Two surfaces of the films

- Top Right - Reconstructed top surface and the glass substrate of the measured sample
- Bottom right - Reconstructed bottom surface of the film and the glass substrate

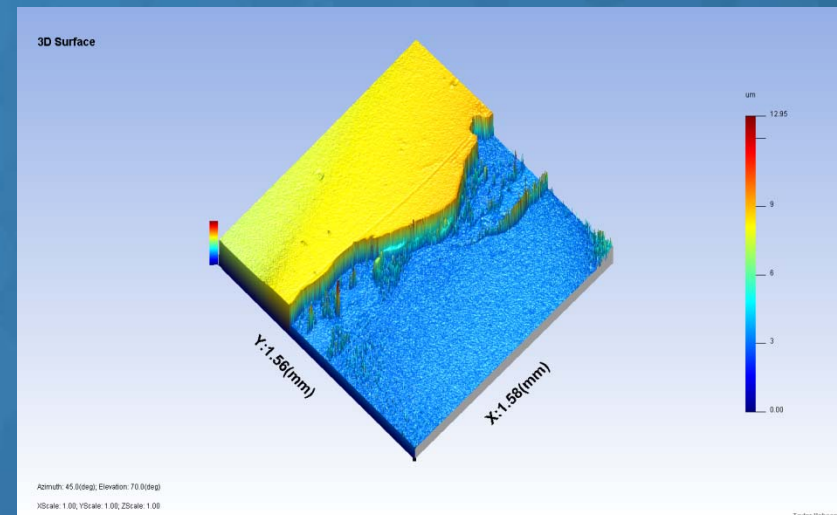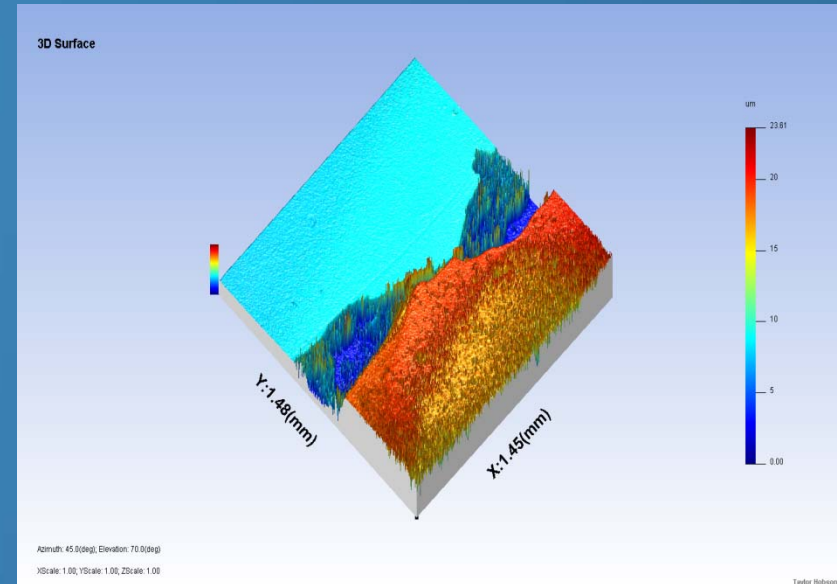


The top surface of the film


- A cross section of the measurement shows the measured step height at the section is 11.0um

Sq=81.7nm

SURFSTAND
2D Profiles Analysis

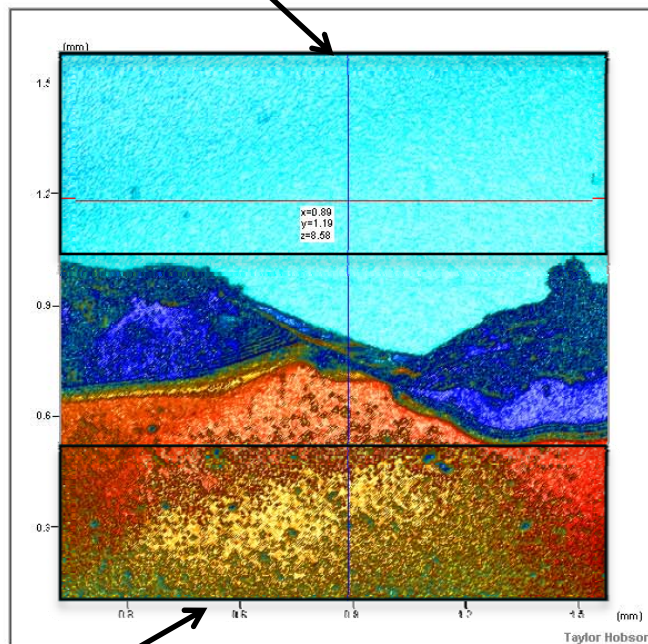

Sq=1.29um

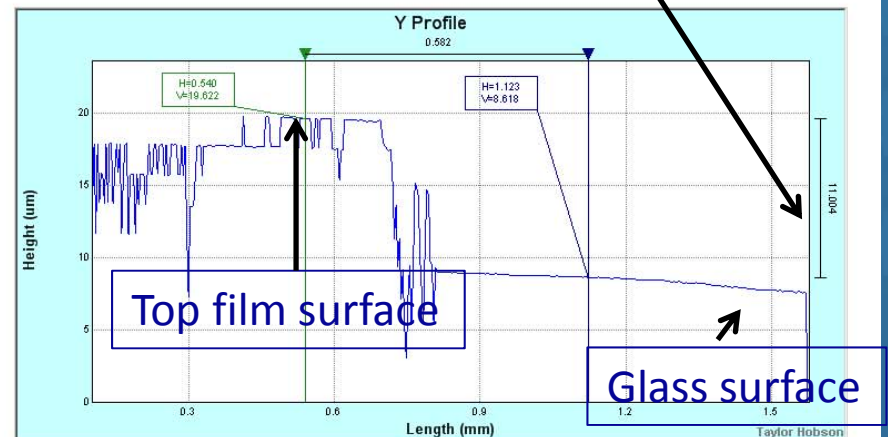


The bottom surface of the film



- A cross section of the measurement shows the measured step height at the section is $-6.66\mu\text{m}$

Sq=56.9nm

SURFSTAND
2D Profiles Analysis


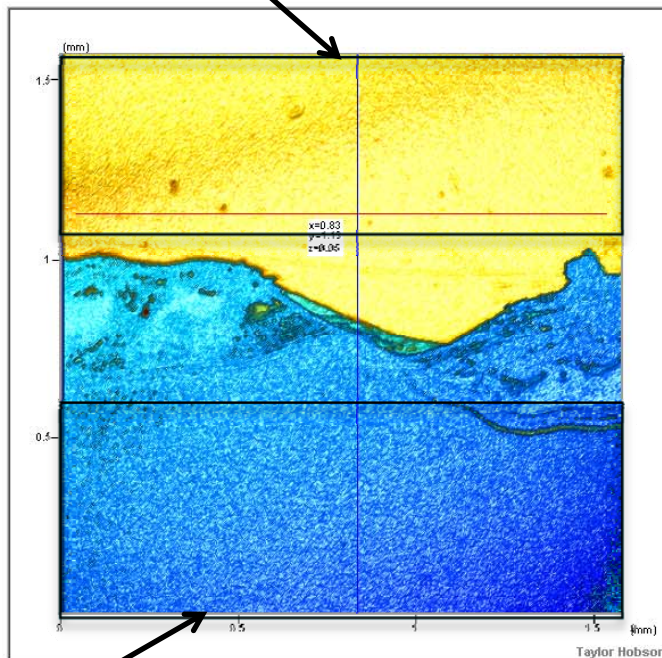


Sq=29.2nm

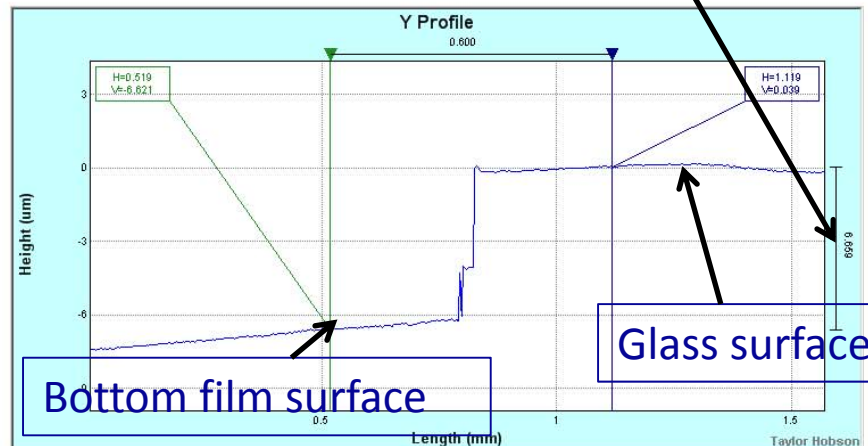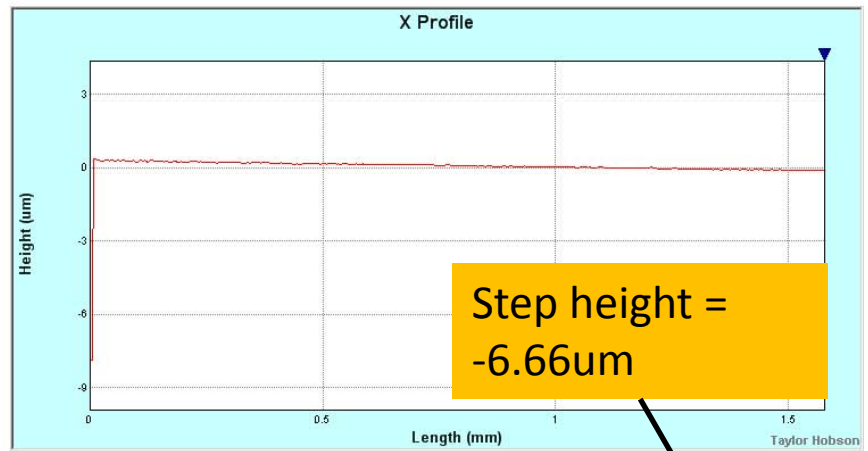


Measurement on the same samples using CCI

- Right - Measured image on the edge of the 10 μm film on microscopic glass substrate
- Bottom - Profile of a cross section of measurement

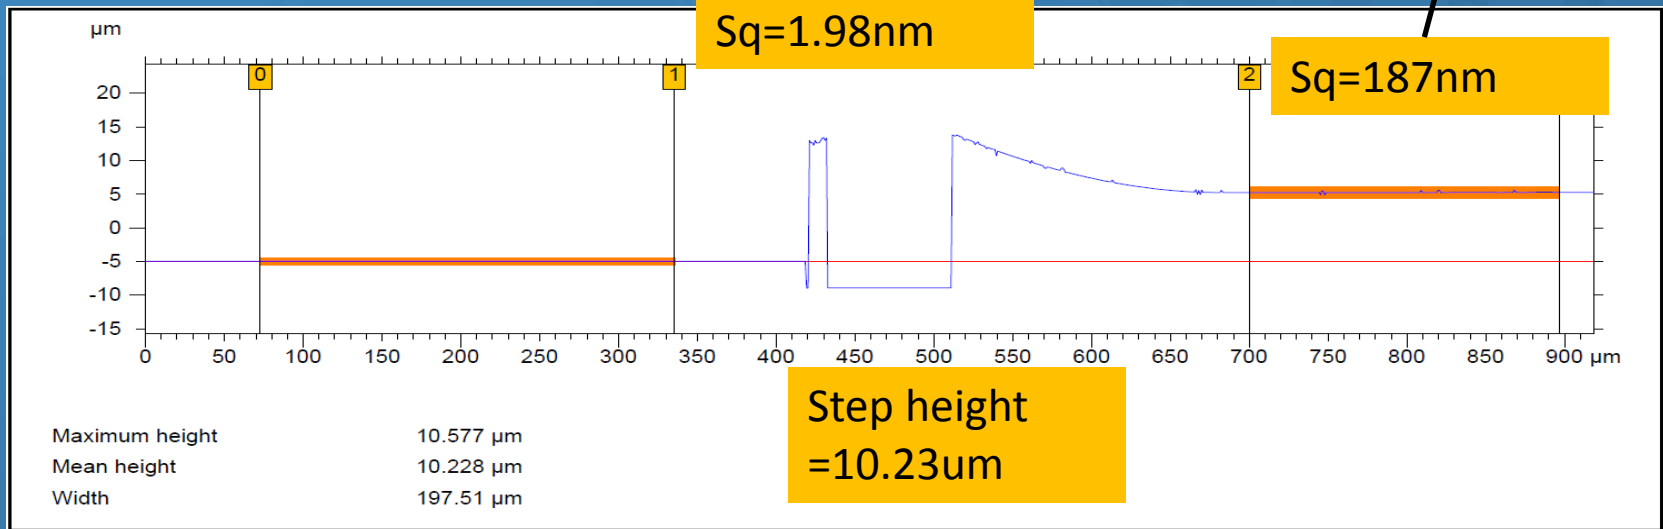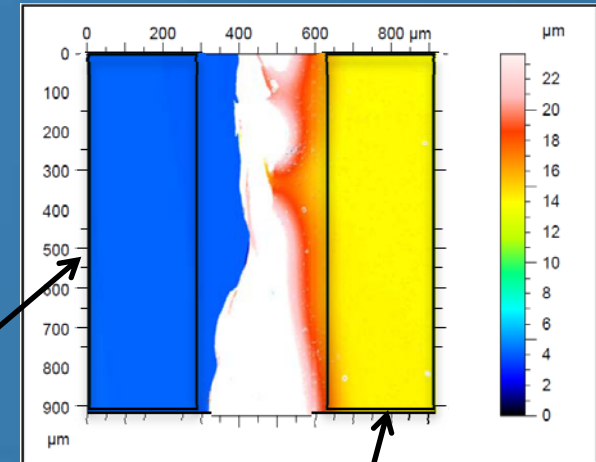

Proposed full field scanning wavelength interferometry system

- A full field scanning wavelength interferometry system has the potential for imaging most of the pellet by arranging an array comprising several wavelength scanning interferometers to image a larger area. Advanced 3D data-stitching and fitting techniques would then need to be applied to provide a more complete surface model.

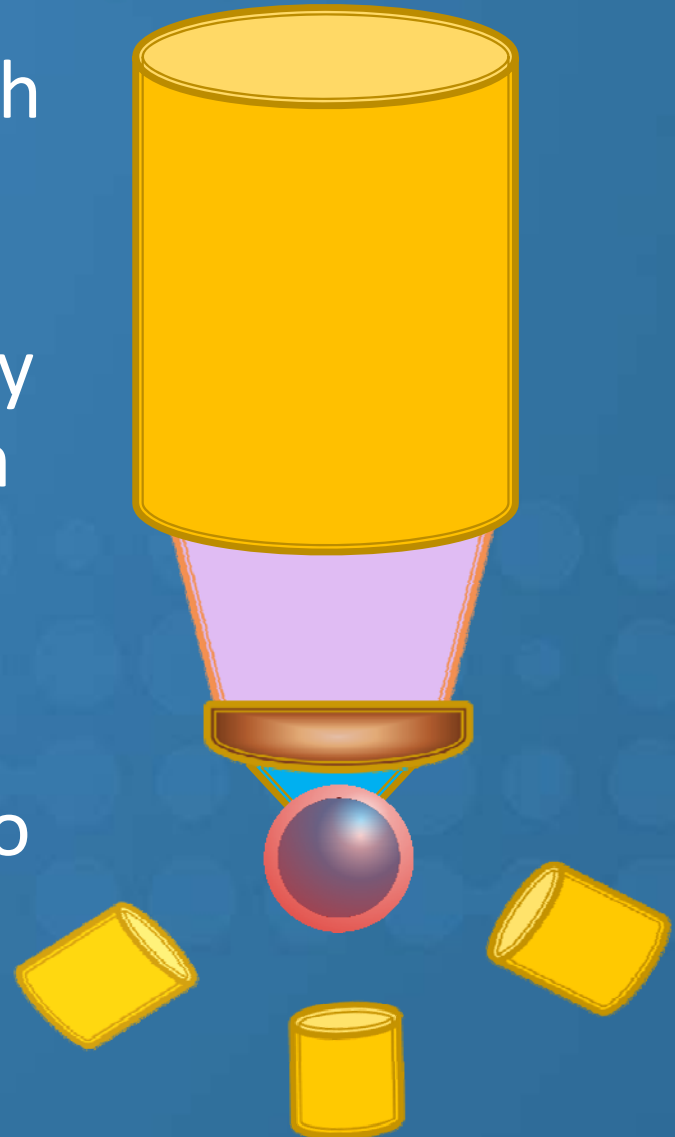

Conclusion

- The study shows the scanning wavelength interferometry is able to measure both the top and the bottom surfaces as well as the thickness of Parylene N film.
- It is possible to measure multi-layer films.
- Improvements are needed to achieve a reliable measurement
 - A better light source for longer coherence length and intensity
 - A none 50:50 ration beam splitter to improve interference signals
 - Improvement on characterisation algorithms

Thanks!

